

CONFIRMATION

Notification: 0000081157_00_02
on changes according to EN 15267 regarding certificate 0000081157_00 dated 5 September 2023

AMS designation: EDM 280 for PM₁₀ and PM_{2.5}

Manufacturer: Grimm Aerosol Technik GmbH
Vordere Aue 4
06774 Muldestausee / OT Friedersdorf
Germany

German Federal Environmental Agency (UBA)

**Announcement regarding the uniform practice in
monitoring emissions and ambient air
dated 27 August 2025
Publication: BAnz AT 31.10.2025 B5**

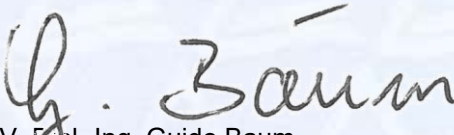
**IV. Notifications as regards the uniform practice in monitoring
emissions and ambient air:**

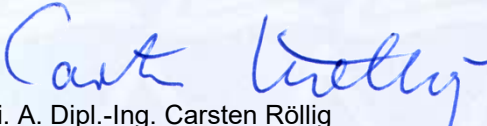
**40 Notification as regards Federal Environment Agency (UBA) notices
of 5 July 2023 (BAnz AT 02.08.2023 B7, chapter II number 1.1) and
of 2 April 2025 (BAnz AT 19.05.2025 B3, chapter IV notification 58)**

The Field Test Kit (FTK) can be used as an option for checking the calibration of the EDM 280 measuring device for PM_{2.5} and PM₁₀ suspended particulate matter from Grimm Aerosol Technik on site/in the field. The test aerosol can be applied using the Field Test Kit (FTK) to the entire system (including the sampling tube) or directly to the measuring insert. If the calibration check using the Field Test Kit (FTK) is positive, it is not necessary to send the measuring insert to Grimm Service or an authorised Grimm service partner every 12 months. The measuring device can now also be equipped and operated with a 2.785 m long sampling tube.

Statement issued by TÜV Rheinland Energy & Environment GmbH dated 20 May 2025

TÜV Rheinland Energy & Environment GmbH
Cologne, 21 November 2025


i. V. Dipl.-Ing. Guido Baum


i. A. Dipl.-Ing. Carsten Röllig

www.umwelt-tuv.eu
qa11-info@tuv.com
Tel. +49 221 806-5200

TÜV Rheinland Energy & Environment GmbH
Am Grauen Stein
51105 Cologne

Test institute accredited to EN ISO/IEC 17025 by DAkkS (German Accreditation Body).
This accreditation is limited to the accreditation scope defined in the enclosure to the certificate D-PL-11120-02-00.