

CONFIRMATION

Notification: 0000035015_04_02
on changes according to EN 15267 regarding certificate 0000035015_04 dated 16 February 2022

AMS designation: MERCEM 300Z / indoor for Hg

Manufacturer: SICK AG
Gisela Sick Straße 1
79276 Reute
Germany

German Federal Environmental Agency (UBA)

**Announcement regarding the uniform practice in
monitoring emissions and ambient air
dated 21 February 2023
Publication: BAnz AT 20.03.2023 B6**

**IV. Notifications as regards the uniform practice in monitoring
emissions and ambient air:**

**40 Notification as regards Federal Environment Agency (UBA) notices
of 12 February 2013 (BAnz AT 05.03.2013 B10, chapter I number 2.3) and
of 28 June 2022 (BAnz AT 28.07.2022 B4, chapter III notification 27)**

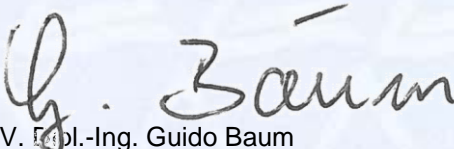
For the MERCEM300Z and MERCEM300Z Indoor measuring system for Hg
from SICK AG, a test cuvette integrated in the analyzer can be used in future
as an option for automatic span point checking and adjustment.

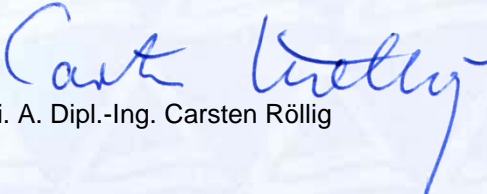
As before, a suitable mercury generator with oxidized mercury must be used
for the QAL 3.

In addition to the optional internal CALSIC test gas generator, the CALSIC N variant
can also be used.

Statement issued by TÜV Rheinland Energy GmbH dated 16 September 2022

TÜV Rheinland Energy GmbH
Cologne, 25 April 2023


i. V. Dipl.-Ing. Guido Baum


i. A. Dipl.-Ing. Carsten Röllig

www.umwelt-tuv.eu
TRE@umwelt-tuv.eu
Tel. +49 221 806-5200

TÜV Rheinland Energy GmbH
Am Grauen Stein
51105 Cologne

Test institute accredited to EN ISO/IEC 17025 by DAkkS (German Accreditation Body).
This accreditation is limited to the accreditation scope defined in the enclosure to the certificate D-PL-11120-02-00.